



Pie Charts

Needle-Devices

3a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "throughout the facility"

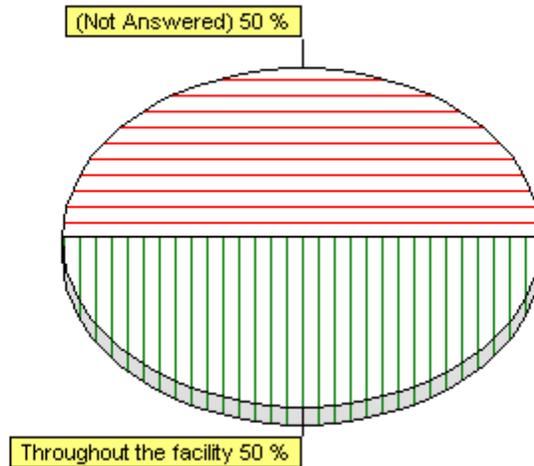


4a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

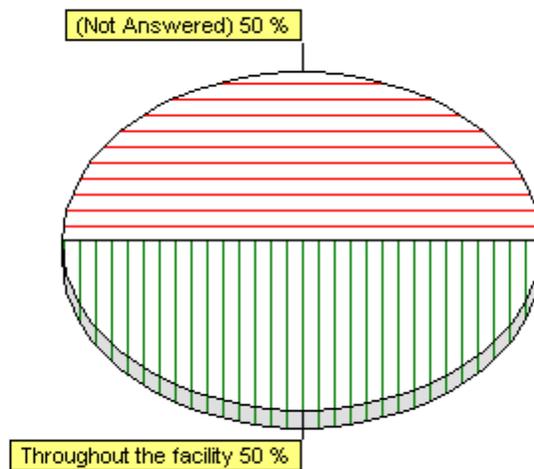


Pie Charts

Needle-Devices

5a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

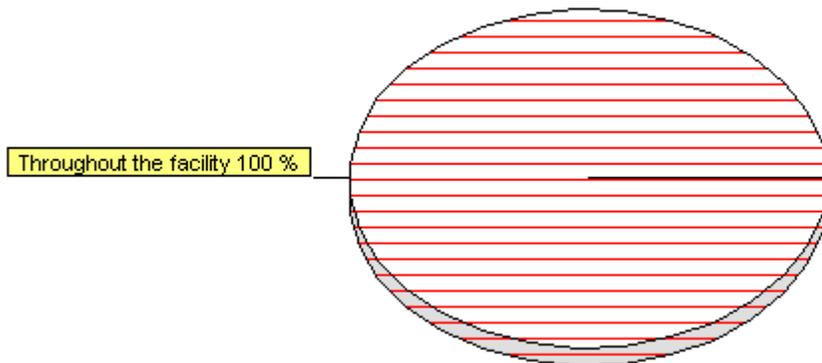


6a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

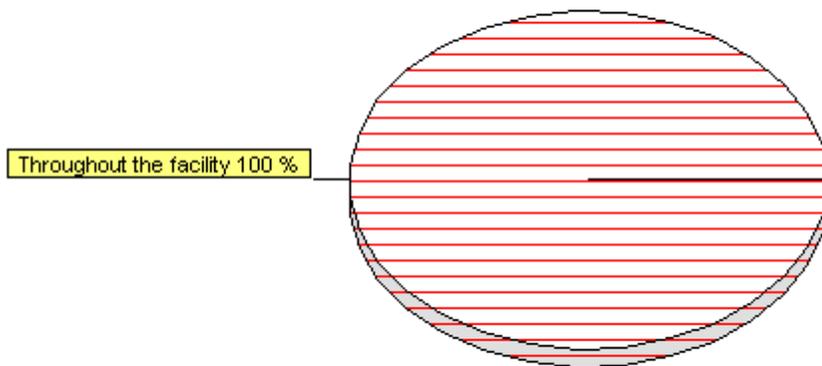


Pie Charts

Needle-Devices

7a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

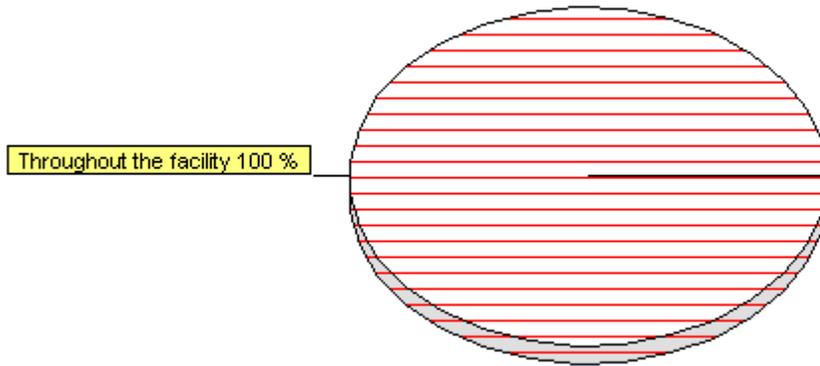


8a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

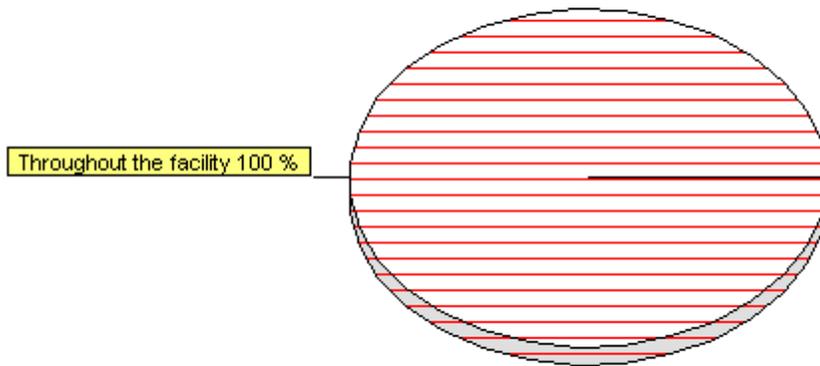


Pie Charts

Needle-Devices

9a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

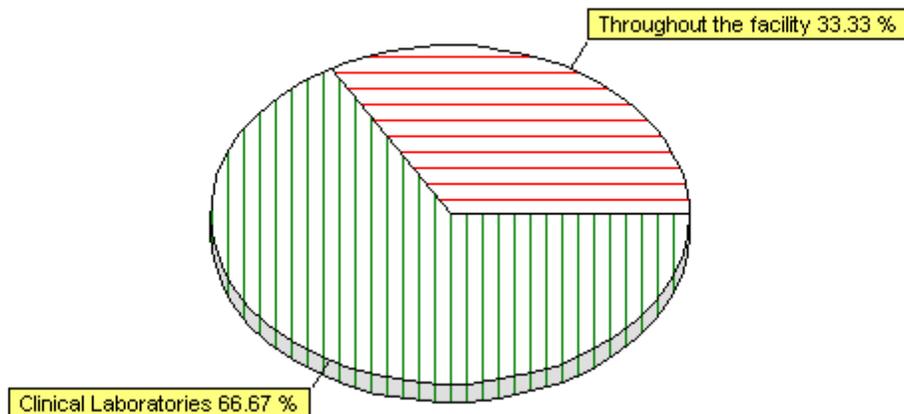


11a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the facility"

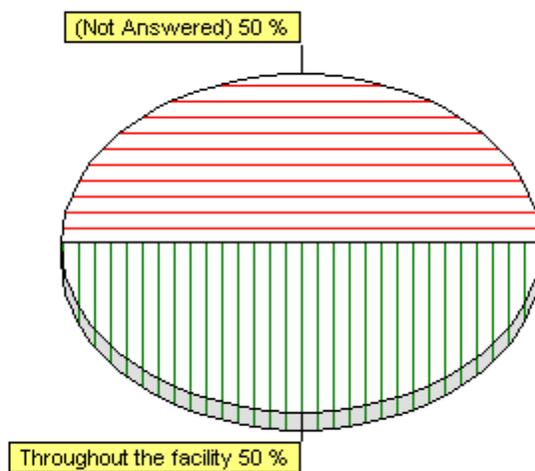


Pie Charts

Needle-Devices

13a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the fa

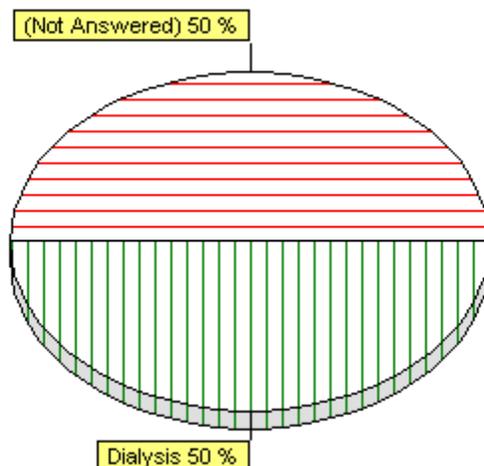


14a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the fa

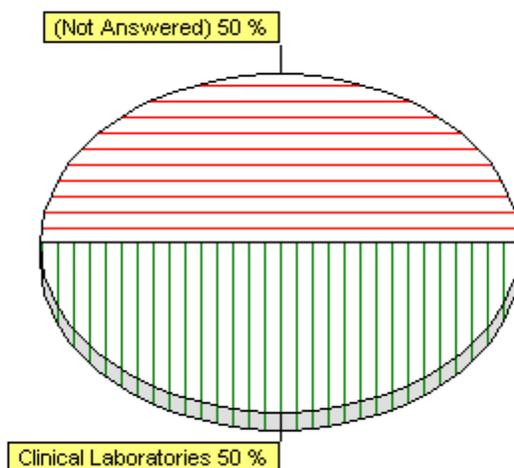


Pie Charts

Needle-Devices

15a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the fa

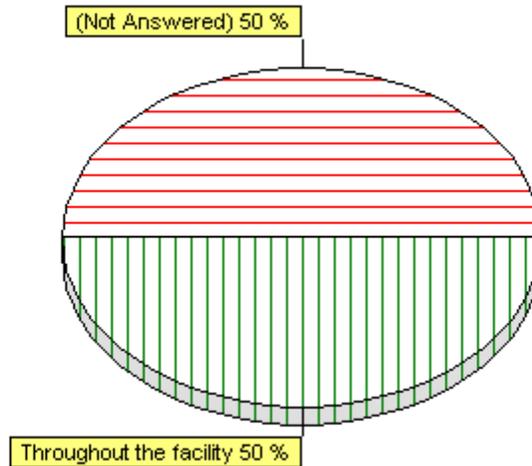

16a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the fa

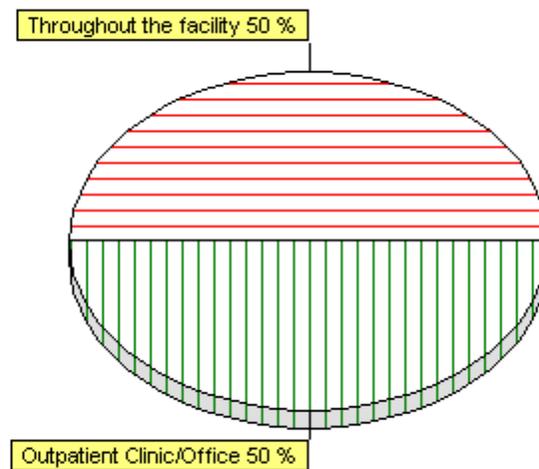

Pie Charts

Needle-Devices

17a. Is the device listed above used throughout the facility or only in high risk locations as defined by the facility? Check "Throughout the fa

